

santex® anatomic

The instruction below should be used in conjunction with detailed information on the packaging.

Short description of the product

Natural rubber latex examination and protective gloves, powder-free / powdered, non-sterile, for disposable use

Full description of the product

Reference numbers	: RD10247060 – 090; RD11247060 – 090
Raw material	: Natural rubber latex
Cuff	: beaded
Colour	: creamy
Shape	: anatomic, hand specific
Size range	: 6.0; 6.5; 7.0; 7.5; 8.0; 8.5; 9.0
AQL	: 1.5
Quantity in packaging	: 2 x 50 pcs. by weight
Shelf life	: 5 years (from the date of manufacturing)

Storage instructions

It is recommended to store the gloves in dry place, in the temperature of 5-35°C and to protect them against direct sunlight and fluorescent light. Keep the gloves in a distance of not less than 1m from heating devices, sources of fire and ozone. Do not keep in direct vicinity of solvents, oils, fuels and lubricants.

MDR classification & compliance

Gloves are classified as class I according to Annex VIII of the Regulation (EU) 2017/745 and comply to standards: EN 455-1:2000, EN 455-2:2009+A2:2013, EN 455-3:2006, EN 455-4:2009, EN ISO 15223-1:2016, EN 1041:2008.

**PPER classification & compliance**

Gloves are category I Personal Protective Equipment as per Annex I of the Regulation 2016/425 and comply to standards: EN 420:2003+A1:2009.

Declaration of Conformity can be found under below web address:

<https://mercatormedical.eu/products/gloves/examination-and-protective-gloves/santex-anatomic-PF>

<https://mercatormedical.eu/products/gloves/examination-and-protective-gloves/Santex-anatomic-PP>

Intended use

These are non-sterile examination and protective gloves for single use, intended for use in medical field to: protect patient and user from cross-contamination, conducting medical examinations, diagnostic and therapeutic procedures and for handling medical contaminated material. Gloves are classified as Medical Devices Class I and as a Personal Protective Equipment Category I. Their design and labelling corresponds to the requirements of the European Regulation 2017/745 on Medical Device and the European Regulation 2016/425 on Personal Protective Equipment. Gloves should be used solely according to their intended application.

Precautions and indications for use

Dry hands before putting the gloves on. Before usage, inspect the gloves for any defect or imperfections. Use at least 1 pair of gloves for one patient and one procedure, these are disposable gloves. When protection is limited to part of the hand only. Do not let chemical substances get under the gloves through the cuff. If a chemical substance reaches the skin, wash it away immediately with plenty of water with soap. If the gloves get punctured, torn or broken during their use, take them off and put on the new ones. Avoid using gloves dirty in the inside as they may cause irritation leading to skin inflammation or more serious damages. The gloves should not be used in contact with open fire and to protect against any sharp tools. The gloves are not intended for welding, electric shock protection, ionizing radiation or from the effect of hot or cold objects.

Components / hazardous components

Some gloves may contain components known to be a possible cause of allergy for person allergic to them, who may develop contact irritation and/or allergic reaction. Gloves made from natural rubber latex may cause allergic reactions, including anaphylactic responses. In case of an allergic reaction, seek medical assistance immediately.

Disposal

Used gloves can be contaminated with contagious or other hazardous substances. They should be disposed of in accordance with local regulation. Gloves should be buried or burned under controlled conditions.


Manufacturer

MERCATOR MEDICAL S.A.
ul. H. Modrzejewskiej 30
31-327 Cracow, Poland
www.mercatormedical.eu


Symbols used on the packaging

MD	Medical device	PPE	Personal Protective Equipment		Powdered gloves
	Do not re-use / gloves are intended for single use		Keep away from moisture, store in a dry place		Powder free gloves
	Non-sterile gloves		Keep away from solar and fluorescent light		Presence of polymer coating on the inner surface of the glove
LOT	Lot / batch number		Temperature limitation / gloves store in temperature 5-35°C		Presence of cosmetic coating on the inner surface of the glove
REF	Catalogue number		Keep away from ozone		Presence of external texture on the glove
EC REP	EU Authorised Representative, symbol should be accompanied by name and address of Authorised Representative		Date of manufacture		Gloves made from nitrile
	Expiry date		Manufacturer, symbol should be accompanied by name and address of Manufacturer		Gloves made from vinyl
ISO 374-5:2016	Marking of gloves protecting against bacteria and fungi		Food contact symbol (article is suitable for food contact, for details check the instruction for use)		Raw material – natural rubber latex
	Marking of gloves protecting against viruses, bacteria and fungi		Package made from paper, qualify for recycling		50 gloves by weight
ISO 374-5:2016			Package is treated as municipal waste		100 gloves by weight
	Marking of type A chemical resistant gloves. Six tested chemicals shall be identified by their code letter under pictogram		Consult instructions for use		200 gloves by weight
VIRUS ISO 374-1:2016/Type A			Additonal information on inner side of package		Do not use, if package is damaged
	Marking of type B chemical resistant gloves. Three tested chemicals shall be identified by their code letter under pictogram		Indicates compliance with the requirements of Ukrainian market		
UVWXYZ ISO 374-1:2016/Type B					
	Marking of type C chemical resistant gloves. One tested chemicals shall be identified by their code letter under pictogram				
XYZ ISO 374-1:2016/Type C					
	Indicates compliance with the requirements of Russian market				
PG					

■ HOW TO PUT THE GLOVES ON?

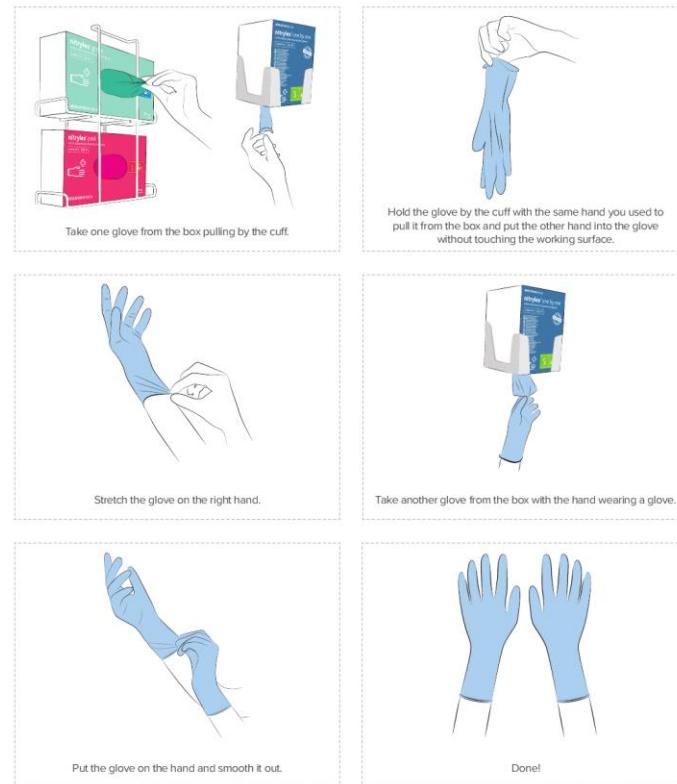

■ HOW TO TAKE THE GLOVES OFF?

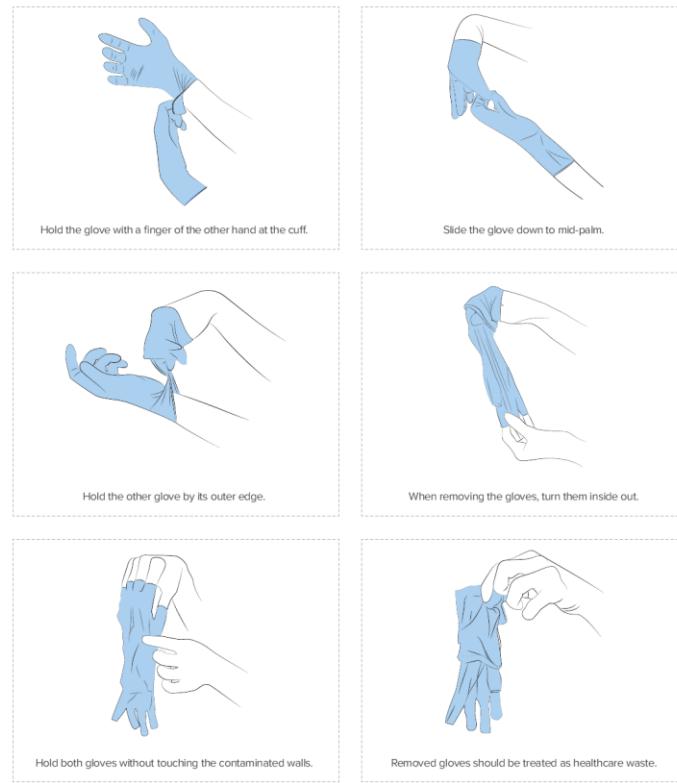



santex® anatomic

Níže uvedené instrukce by měly být používány ve spojení s detailními informacemi na obalu.

Krátka popis produktu

Latexové vyšetřovací a ochranné rukavice, nepudrované / pudrované, nesterilní, jednorázové.

Popis produktu

Referenční čísla	: RD10247060 – 090; RD11247060 – 090
Materiál	: latex
Manžeta	: rolovaná
Barva	: krémová
Tvar	: anatomické, specifické pro levou a pravou
Velikosti	: 6.0; 6.5; 7.0; 7.5; 8.0; 8.5; 9.0
AQL	: 1.5
Množství v balení	: 2 x 50 ks dle váhy
Záruka kvality	: 5 let (od data výroby)

Pokyny k uchovávání

Je doporučeno uchovávat tyto rukavice na suchém místě, při teplotě v rozmezí 5-35 °C a chránit je před přímým slunečním zářením a fluorescenčním světlem.

Rukavice udržujte ve vzdálenosti nejméně 1 m od topných zařízení, zdrojů ohně a ozónu.

Neskladujte v přímé blízkosti rozpouštědel, olejů, paliv a maziv.

MDR klasifikace & shody

Rukavice jsou klasifikované jako zdravotnický prostředek třídy I podle přílohy VIII Nařízení (EU) 2017/745 a splňují standardy:

EN 455-1:2000, EN 455-2:2009+A2:2013, EN 455-3:2006, EN 455-4:2009, EN ISO 15223-1:2016, EN 1041:2008.



OOP klasifikace & shody

Rukavice jsou v kategorii I osobních ochranných prostředků podle přílohy I Nařízení 2016/425 a odpovídají standardům: EN 420:2003+A1:2009.

Prohlášení o shodě je na webové adrese:

<https://mercatormedical.eu/products/gloves/examination-and-protective-gloves/santex-anatomic-PF>

<https://mercatormedical.eu/products/gloves/examination-and-protective-gloves/Santex-anatomic-PP>

Účel použití

Tyto rukavice jsou nesterilní vyšetřovací a ochranné rukavice na jedno použití, určené pro použití ve zdravotnickém prostředí za účelem: ochrany pacienta a uživatele před křížovou kontaminací, provádění lékařských vyšetření, diagnostických a terapeutických postupů a manipulace se zdravotně kontaminovaným materiálem. Rukavice jsou klasifikované jako zdravotnický prostředek třídy I a jako osobní ochranný prostředek kategorie I. Jejich design a označení je v souladu s požadavky Evropské směrnice o zdravotnických prostředcích 2017/745 a Evropským nařízením 2016/425 o osobních ochranných prostředcích. Rukavice by měly být používány pouze v souladu s jejich zamýšleným použitím.

Opatření a návod k použití

Před nasazením rukavic si osušte ruce. Před použitím zkontrolujte rukavice, zda nejsou poškozené nebo vadné. Použijte alespoň jeden páru rukavic na jednoho pacienta a jednu proceduru, rukavice jsou jednorázové. Zabraňte proniknutí chemických látek pod rukavice přes manžetu. V případě, že se chemická látka dostane na pokožku, ihned ji omyjte velkým množstvím vody s mýdlem. Pokud se rukavice během používání propichnou, roztrhnou nebo protrhnou během používání, sundejte je a použijte nové. Ve vnitřním prostoru nepoužívejte špinavé rukavice, protože by mohly způsobit podráždění, které by mohlo způsobit zánět kůže nebo vážnější poškození. Rukavice by neměly být používány v kontaktu s otevřeným ohněm a jako ochrana před ostrými nástroji. Rukavice nejsou určeny ke svařování, jako ochrana před elektrickým proudem, ionizujícím zařízením ani před působením horkých nebo studených předmětů.

Komponenty/nebezpečné komponenty

Některé rukavice mohou obsahovat složky, známé možností způsobit alergii osobám na ně alergickým, která se může rozvinout v kontaktní dráždění a/ nebo v alergickou reakci. Rukavice vyrobené z přírodního kaučukového latexu mohou způsobit alergické reakce, včetně anafylaktických reakcí. V případě alergické reakce okamžitě vyhledejte lékařskou pomoc.

Likvidace

Použité rukavice mohou být kontaminovány infekčními a jinými nebezpečnými materiály a mělo by s nimi být zacházeno jako se zdravotnickým odpadem. Rukavice by měly být skladkovány nebo spáleny za kontrolovaných podmínek.

Výrobce

MERCATOR MEDICAL S.A.

ul. H. Modrzejewskiej 30

31-327 Krakov, Polsko

www.mercatormedical.eu



Symboly použité na balení

	Zdravotnický prostředek		Osobní ochranný prostředek		Pudrované rukavice
	Nepoužívejte opakovaně / rukavice jsou určeny k jednorázovému použití		Udržujte suché		Nepudrované rukavice
	Nesterilní rukavice		Udržujte od slunečního záření a fluorescenčního světla		Přítomnost polymerního povlaku na vnitřním povrchu rukavic
	Lot / číslo šarže		Omezení teploty / uchovávejte rukavice při teplotě 5-35 °C		Přítomnost kosmetického povlaku na vnitřním povrchu rukavic
	Katalogové číslo		Držte stranou od ozónu		Přítomnost vnější textury na rukavice
	Zplnomocněný zástupce EU, symbol by měl být doplněn jménem a adresou zplnomocněného zástupce		Datum výroby		Nitrilové rukavice
	Datum expirace		Výrobce, tento symbol je používán společně se jménem a adresou výrobce		Vinylové rukavice
	Označení rukavic ochraňujících před bakteriem a plísním		Symbol styku s potravinami (výrobek je vhodný pro styk s potravinami, podrobnosti viz návod k použití).		Latexové rukavice
	Označení typu A chemicky odolných rukavic. Šest testovaných chemikálií se označí kódovým písmenem pod piktogramem.		Balení vyrobeno z papíru, vhodné pro recyklaci		50 rukavic dle váhy
	Označení typu B chemicky odolných rukavic. Tři testované chemikálie se označí kódovým písmenem pod piktogramem.		Balení je považováno za komunální odpad		100 rukavic dle váhy
	Označení typu C chemicky odolných rukavic. Jedna testovaná chemikálie se označí kódovým písmenem pod piktogramem.		Balení je považováno za komunální odpad		200 rukavic dle váhy
	Označuje shodu s nařízením ruského trhu		Další informace na vnitřní straně balení		Nepoužívejte, je-li balení poškozeno
			Označuje shodu s nařízením ukrajinského trhu		

**■ HOW TO PUT THE GLOVES ON?**

Take one glove from the box pulling by the cuff.



Hold the glove by the cuff with the same hand you used to pull it from the box and put the other hand into the glove without touching the working surface.



Stretch the glove on the right hand.



Take another glove from the box with the hand wearing a glove.



Put the glove on the hand and smooth it out.



Done!

■ HOW TO TAKE THE GLOVES OFF?

Hold the glove with a finger of the other hand at the cuff.



Slide the glove down to mid-palm.



Hold the other glove by its outer edge.



When removing the gloves, turn them inside-out.



Hold both gloves without touching the contaminated walls.



Removed gloves should be treated as healthcare waste.